Propaq® LT Vital Signs Monitor
Quick Reference

Neonate — Birth through 28 days, or 44 weeks gestational
Pediatric — 29 days through 12 years
Adult — 13 years and older

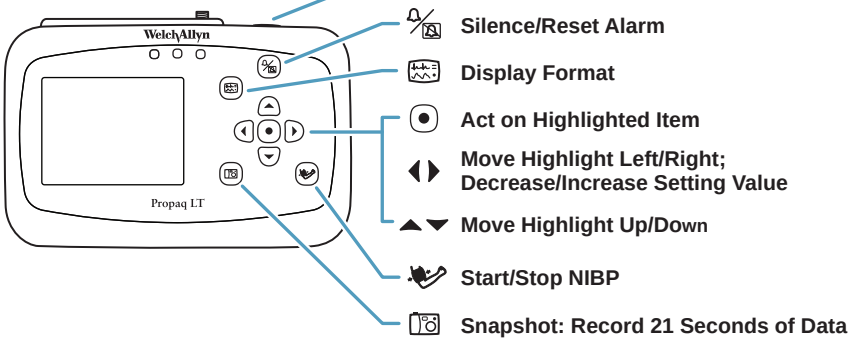

Change Alarm Limits
(HR/PR, NIBP, SpO_2, Resp)
(select) ● (select parameter) (change limits) ●

Change Alarm Tone
(Low, Medium, High)
(SpO2) ● Setup ● Alarms - Alarm Tone ● (select) ●

Silence/Reset Alarm Tone

Suspend Alarm Tones
(HR/min) ● Setup ● Alarms - Suspend Audible Alarms ● (select) ●

Change (Vital Sign) Settings
(HR/PR, NIBP, SpO_2, Resp)
(select) ● (parameter)

Change Patient Mode
(Adult, Pediatric, Neonate)
Adult ● (select) ●

Change Lead
(I, II, III, ...)
II ● (select)

Set NIBP mode
(Auto, Manual, Turbo)
NIBP mmHg ● NIBP Mode (select) ●

Change Monitor Setup
(Alarms, ECG, NIBP, ...)
(NIBP) ● Setup ● (select) ● (set values)

Change time/date
(Hour, Minute, Month, ...)
xx:xx:xx ● (select) (change) ●

View Trends
(NIBP) ● Trends ●

View Snapshots
(HR/min) ● Snapshots ●

Welch Allyn • Beaverton, Oregon USA
©2005 • Printed in USA • P/N: 810-1819-00 Rev. B 03/06

800 289 2500
503 530 7500

Welch Allyn®